

Methods, quality control and specimen management in an international multicentre investigation of type 1 diabetes: TEDDY

Kendra Vehik^{1*} Steven W. Fiske¹ Chad A. Logan¹
Daniel Agardh² Corrado M. Cilio² William
Hagopian³ Olli Simell⁴ Merja Roivainen⁵ Jin-Xiong
She⁶ Thomas Briese⁷ Sami Oikarinen⁸ Heikki
Hyoty^{8,9} Anette-G. Ziegler¹⁰ Marian Rewers¹¹ Ake
Lernmark² Beena Akolkar¹² Jeffrey P. Krischer¹
Brant R. Burkhardt^{1,13} The TEDDY Study Group

¹Pediatrics Epidemiology Center, Morsani College of Medicine, University of South Florida, Tampa, FL, USA

²Department of Clinical Sciences, Malmo University Hospital, Lund University, Malmo, Sweden

³Pacific Northwest Diabetes Research Institute, Seattle, WA, USA

⁴Department of Pediatrics, University of Turku, Turku, Finland

⁵National Institute for Health and Welfare, Helsinki, Finland

⁶Medical College of Georgia, Augusta, GA, USA

⁷Center for Infection and Immunity, Mailman School of Public Health, Columbia University, New York, NY, USA

⁸Department of Virology, Medical School, University of Tampere, Tampere, Finland

⁹Department of Clinical Microbiology, Centre of Laboratory Medicine, Tampere University Hospital, Tampere, Finland

¹⁰Institute of Diabetes Research, Helmholtz Zentrum München and Forschergruppe Diabetes e.V., Neuherberg, Germany

¹¹Barbara Davis Center for Childhood Diabetes, University of Colorado Denver, Aurora, CO, USA

¹²Division of Diabetes, Endocrinology and Metabolic Diseases, National Institute of Diabetes and Digestive and Kidney Diseases, National Institutes of Health, Bethesda, MD, USA

¹³Department of Cell Biology, Microbiology and Molecular Biology, University of South Florida, Tampa, FL, USA

*Correspondence to: Kendra Vehik, Pediatrics Epidemiology Center, Morsani College of Medicine, University of South Florida, 3650 Spectrum Blvd., STE 100, Tampa, FL 33612, USA.
E-mail: kendra.vehik@epi.usf.edu

Received: 17 September 2012

Revised: 24 April 2013

Accepted: 7 May 2013

Abstract

Background The vast array and quantity of longitudinal samples collected in The Environmental Determinants of Diabetes in the Young study present a series of challenges in terms of quality control procedures and data validity. To address this, pilot studies have been conducted to standardize and enhance both biospecimen collection and sample obtainment in terms of autoantibody collection, stool sample preservation, RNA, biomarker stability, metabolic biomarkers and T-cell viability.

Research Design and Methods The Environmental Determinants of Diabetes in the Young is a multicentre, international prospective study ($n = 8677$) designed to identify environmental triggers of type 1 diabetes (T1D) in genetically at-risk children from ages 3 months until 15 years. The study is conducted through six primary clinical centres located in four countries.

Results As of May 2012, over three million biological samples and 250 million total data points have been collected, which will be analysed to assess autoimmunity status, presence of inflammatory biomarkers, genetic factors, exposure to infectious agents, dietary biomarkers and other potentially important environmental exposures in relation to autoimmunity and progression to T1D.

Conclusions Detailed procedures were utilized to standardize both data harmonization and management when handling a large quantity of longitudinal samples obtained from multiple locations. In addition, a description of the available specimens is provided that serve as an invaluable repository for the elucidation of determinants in T1D focusing on autoantibody concordance and harmonization, transglutaminase autoantibody, inflammatory biomarkers (T-cells), genetic proficiency testing, RNA lab internal quality control testing, infectious agents (monitoring cross-contamination, virus preservation and nasal swab collection validity) and HbA_{1c} testing. Copyright © 2013 John Wiley & Sons, Ltd.

Keywords quality control; data integrity; stool sample preservation; RNA; biomarker stability; metabolic biomarkers; T-cell viability

Introduction

The advent of multicentre studies has necessitated more rigorous quality control (QC) methods to minimize interlaboratory and intercentre variation across

highly diverse locations. Extended longitudinal observational study designs add an additional layer of complexity with a high volume of repeated data collected over long periods. The Environmental Determinants of Diabetes in the Young (TEDDY) is a unique 15-year longitudinal observational study that spans four countries and 12 clinical sites. This study is setting the benchmark for analysing many environmental exposures as markers for environmental and lifestyle factors and their association with type 1 diabetes (T1D) [1]. QC efforts at the initiation of the study were necessary to assess the reliability and validity of data/sample collection, shipping and analyses given the sheer number of biospecimens collected from widespread clinical centres for analysis in multiple core laboratories. Because onset of T1D is believed to be the result of a multifactorial process of dynamic interaction of both genetic susceptibility and environmental triggers, the objective of the TEDDY study is to identify environmental factors (viruses, bacteria, diet, lifestyle, stress and chemical exposures) associated with islet autoimmunity and T1D. To accomplish this difficult objective, a long-term prospective observational study was initiated in a high genetic risk cohort. In addition, the study will assess factors associated with celiac disease.

This article summarizes the technical aspects of the QC methods employed for ensuring accurate human leukocyte antigen (HLA) screening across clinical centres, autoantibody assay harmonization across core laboratories, stool sample collection, shipment and preservation, RNA quality, biomarker stability, T-cell viability and data quality. The TEDDY study plans to explore novel data-driven approaches to identify phenotypes linked to T1D susceptibility related to metabolomics, the microbiome, viral metagenomics, epigenetics and gene expression. Biospecimens are stored at the TEDDY Repository managed by Fisher Biosciences. A detailed summary of the available biospecimens collected to assist in the identification of gene–environment interactions associated with T1D and celiac disease is provided in this article.

Study design and population

The Environmental Determinants of Diabetes in the Young is a multicentre, multinational epidemiological natural history study initiated by the National Institutes of Health (NIH) to identify environmental exposures associated with autoimmunity and T1D onset in children at increased HLA-conferred genetic risk for this disease [1]. Newborn screening began in September 2004 and was completed in March 2011. There are 8677 children enrolled in the 15-year prospective follow-up. There are four countries and 12 centres in Europe (Finland, Germany and Sweden)

and the USA (Georgia/Florida, Colorado and Washington) and the central TEDDY Data Coordinating Center (DCC) in Tampa, Florida. The TEDDY study cohort analysis plan incorporates two different statistical designs depending on the nature of the factor under study. For exposures whose values are known on the entire cohort, a prospective design utilizing survival analysis (log-rank tests and Cox proportional hazards models), repeated measures analysis of variance, generalized estimating equations and general linear models will be used. For factors related to sample assays, a nested case–control design will be employed. The matched case–control study using conditional logistic regression will involve two interim phases of analysis at 5 and 10 years and the final analysis at the end of the study. The TEDDY study has entered the first phase of interim analyses with 114 T1D cases and 418 subjects with persistent confirmed autoantibodies with a 1:3 case–control match for the majority of biological samples and a 1:1 match for gene expression, the microbiome and viral metagenomics. Clinic visits began at 3 months of age and continued at a 3-month interval up to the age of 4 years. If subjects seroconvert to persistent autoantibody positivity (GADA, IA-2A or mIAA), they continue on the 3-month interval visit schedule up to age 15 years; otherwise, they switch to a 6-month interval visit schedule (Table 1).

Methods and quality control

Genetic inclusion screening quality control

HLA screening at clinical centres with confirmatory testing at a central lab

The TEDDY cohort was enriched for subjects likely to reach disease endpoints by screening for specific HLA genotypes associated with moderate to high future risk of T1D. T1D incidence is relatively low compared with other chronic disease; therefore, TEDDY screened 424,788 children to identify its cohort. A total of 418,367 general population (GP) infants were screened, of which 20,152 (4.8%) were eligible, and 1437 of the 6421 screened infants (22.4%) with a first-degree relative with T1D (FDR) were eligible. The details of this effort have been previously described [2]. The cohort was identified by HLA class II genotyping of newborn screening samples to allow determination of risk based on criteria established with pre-TEDDY data. The HLA typing was completed at five of the six international centres (the Finland Center conducted the typing for the German Center) using either asymmetric polymerase chain reaction and subsequent hybridization of allele-specific probes for HLA-DQA1, DQB1 and DRB1 as described [3]

using Dissociation-Enhanced Lanthanide Fluorescent Immunoassay (DELFI) reagents (Perkin-Elmer, Waltham, MA USA) or a dot blot hybridization assay as detailed elsewhere [4]. Both methods used the same study inclusion criteria. There were separate inclusion criteria for the GP and FDRs of T1D patients. The FDR eligibility includes nine haplotypes (*DR3/4*, *DR4/4*, *DR4/8*, *DR3/3*, *DR4/4b*, *DR4/1*, *DR4/13*, *DR4/9* and *DR3/9*) for broad HLA diversity; whereas, the GP eligibility included only the first four haplotypes with *DRB1*0403* as an exclusion allele. Errors in screening genotyping could originate from sample mislabelling, true genotyping errors or rare haplotypes resulting in inferential errors. Central high-resolution confirmation testing was performed on all enrolled subjects and showed that the low-cost and low-resolution genotyping techniques employed at the screening centres yielded an accuracy of 99%. The TEDDY screening strategy demonstrated that different low-cost and low-resolution genotyping methods can result in efficient and accurate identification of a high-risk cohort for follow-up on the basis of the TEDDY HLA inclusion criteria.

Genetic proficiency testing

The TEDDY study achieved excellent genotyping accuracy using genetic proficiency testing (PT) to ensure high initial and ongoing quality for T1D studies that employ HLA genetic risk assessment [5]. The Centers for Disease Control and Prevention (CDC) conducts both a voluntary quarterly PT programme available to any laboratory and a mandatory annual PT challenge for TEDDY laboratories [5]. To mimic and test genotyping samples as those received by TEDDY, CDC sent whole blood and dried blood spots samples with a wide range of validated HLA-DR and HLA-DQ genotypes to the five participating laboratories conducting screening tests and the centralized data centre. Results were evaluated on the basis of both the reported haplotypes and the HLA genetic risk assessment. In the past 6 years, the voluntary quarterly PT reported from the 24 panels that 94.7% (857/905) of the relevant HLA-DR or HLA-DQ alleles were correctly identified with 96.4% (241/250) correctly categorized for risk assessment. There was significant improvement seen during the time interval of this programme, with correct categorization reaching 100% during the last 3 years. TEDDY PT during the past four evaluations has revealed a genotyping accuracy of 99.9% (1153/1154). The different analytical methods used by T1D research centres have all provided accurate (>99%) results for genetic risk assessment. The two complementary CDC PT programmes have documented the validity of the various approaches for screening and contributed to overall quality assurance.

Autoantibody concordance and harmonization

Autoantibody harmonization

Participants in TEDDY have autoantibodies measured starting at 3 months of age every 3 months until age 4 years, whereby on the basis of the appearance of a single persistent confirmed autoantibody, the participant continues on the 3-month interval or if negative transitions to a 6-month interval until the age of 15 years (Table 1). As of May 2012, serum stored in the TEDDY Repository designated for autoantibody testing has been captured on 78% of the cohort adjusted for lost to follow-up and withdrawn subjects. In an effort to ensure concordance between the two TEDDY core laboratories that process the autoantibody samples [Barbara Davis Center (BDC), Aurora, Colorado and the University of Bristol Laboratory, Bristol, UK], TEDDY participated in the National Institute of Diabetes and Digestive and Kidney Diseases (NIDDK) harmonization project in collaboration with the Diabetes Research Institute in Munich, Germany; the details have been published [6]. To evaluate the impact of the harmonized assay protocol on concordance of IA-2A and GADA results, two laboratories retested stored TEDDY study sera using the harmonized assays. For IA-2A, using a common threshold of 5 DK U/mL, 549 of 550 control and patient samples were concordantly scored as positive or negative; specificity was greater than 99% with sensitivity 64% in all laboratories. For GADA, using thresholds equivalent to the 97th percentile of 974 control samples in each laboratory, 1051 (97.9%) of 1074 samples were concordant. On the retested TEDDY samples, discordance decreased from 4% to 1.8% for IA-2A ($n = 604$ samples; $p = 0.02$) and from 15.4% to 2.7% for GADA ($n = 515$ samples; $p < 0.0001$). The precision of the measurement using the harmonized assay was determined in patient samples with values above 2.5 U/mL. The calibration of NIDDK calibrator samples and the median (interquartile range) of the coefficients of variation for IA-2A in the three laboratories (BDC, Bristol and Munich) were 11.6% (10.6–21.5), 18.8% (15.8–23.9) and 8.7% (6.8–12.9) and for GADA were 10.8% (7.8–17.1), 9.1% (5.2–13.9) and 9% (6–15.3) [6]. The harmonization programme for GADA and IA-2A was found to be feasible using large volume working calibrators and similar protocols. It provides a sound approach to ensure consistency in autoantibody measurements. In addition to the harmonized assay, the TEDDY study confirms all autoantibody positive samples and 5% of all negative samples at both laboratories. External QC is also employed to test concordance by including external control samples identified and aliquoted in Gainesville, Florida and Munich, Germany, embedded in the routine monthly shipments to the two TEDDY core laboratories. These results are

compared with external control reference results from the Munich laboratory.

Transglutaminase autoantibody

Tissue transglutaminase autoantibodies (tGA) are serological markers for celiac disease, a chronic small bowel disease with autoimmune features caused by intolerance to dietary gluten and frequently detected among T1D patients. All children in TEDDY are annually screened for tGA starting at 24 months of age using radiobinding assays analysed in the same two core laboratories as the diabetes autoantibodies. If a child is positive for tGA at 24 months, then all of their earlier samples (3–21 months) are tested for tGA. A child is classified as having persistent tGA when two consecutive measurements drawn at least 3 months apart are both positive. Children identified as persistent tGA in TEDDY are referred to a gastroenterologist for management at the clinical discretion of their primary provider. The decision to perform a biopsy is outside the TEDDY study protocol.

At the BDC, the radiobinding assay uses anti-IgA agarose to capture IgA-tGA, whereas in Bristol, a mixture of both anti-IgA agarose and protein A sepharose (PAS) is used to assess both IgA-tGA and IgG-tGA. Because of the discrepancy in the detection methods of the two IgA-tGA assays [7], TEDDY uses the BDC laboratory as a screen, and the results are based upon the Bristol Laboratory's result. Children with a tGA level >0.05 at the BDC and >1.3 units (U) in Bristol are deemed tGA antibody-positive and are reassayed in a follow-up sample taken after 3 months in samples collected at 24 and 36 months of age and after 6 from 48 months of age. To exclude regional variations in the presence of tGA due to methodological differences between the BDC and Bristol laboratories, persistent tGA-positive sera were analysed in a small set of samples at both laboratories for confirmatory analysis. In all, 900 TEDDY subjects were included for this exchange analysis and revealed a 93% concordance between the tGA assays, where 54 of discordant children were positive only in the Bristol and three in the BDC assays. Among those 54 children first detected in Bristol but not at the BDC, a total of 27 children reverted to tGA-negative after one or two follow-up samples, 17 remained persistent tGA positive of which 10 children had subsequent follow-up samples with high tGA levels and were later diagnosed with celiac disease by their physician.

This finding resulted in a protocol modification in order to harmonize the tGA assays in TEDDY, and it was decided that Bristol would be used as the reference laboratory in TEDDY for future analyses. The majority of discrepant samples were detected in individuals with low positive tGA levels in Bristol and had a tGA level between the detection level 0.01 and cut-off level 0.05 at the BDC. All sera with tGA levels >0.01 at the BDC are now

reassayed at the laboratory in Bristol for confirmation of persistence. Children found to be persistent positive in Bristol are not reassayed at the BDC. In discordant cases, sera are further assayed separately for IgG-tGA by the PAS assay in order to distinguish between IgA-tGA and IgG-tGA positivity. Children with initial discordant sera later confirmed by the PAS assay are defined as persistent IgG-tGA positive.

Inflammatory biomarkers

The Environmental Determinants of Diabetes in the Young plans to evaluate serum proteins and peripheral blood mononuclear cells (PBMC) in high-risk children as markers of inflammation and autoimmunity to identify additional biomarkers and time windows of possible therapeutic intervention for T1D.

Cryopreservation of peripheral blood mononuclear cells

The PBMC sample collection was initiated in May 2010. PBMCs are isolated from TEDDY children at 3-month intervals using cell preparation tubes (CPT) and a freezing protocol derived from the immune tolerance network guidelines [8,9]. To enhance isolated PBMC quality, technicians involved in cryopreservation of PBMCs are required to be annually certified. This certification procedure requires the collection of whole blood in two CPT from three separate non-TEDDY donors and the preservation of PBMCs in three separate vials frozen according to the TEDDY Manual of Operations (MOO). The samples are maintained at -80°C for 2 days before shipment to the central laboratory (Benaroya Research Institute, Clinical Core Lab, Seattle, USA) for QC. Cells are evaluated for viability and recovery by certified technicians. The samples with documented sample volume and count information are shipped to the Benaroya Research Institute for centralized analysis. A passing score is determined by both cell recovery and viability with results reported by the DCC.

To optimize the recovery of PBMCs from CPT, a pilot study was conducted to define the best method for cell isolation and to minimize cell loss following centrifugation. Blood samples from ten healthy donors were collected in three separate CPT, and after centrifugation, PBMC were collected in three different ways: (1) removing the PMBC layer without mixing the cells with the autologous plasma, (2) removing the cells after resuspension in the autologous plasma by gentle pipetting, and (3) collecting cells as outlined earlier but the tubes were further washed twice with 2 mL of Roswell Park Memorial Institute (RPMI) medium [9] to collect residual cells. Cell count and viability were determined by trypan blue exclusion assay with hemocytometer. The results demonstrated that a considerable amount of PBMCs remained in the

CPT post-centrifugation and PBMC recovery was increased from 14% to 88% with inclusion of two additional washes of the CPT sample. Therefore, this improved protocol was added to the TEDDY MOO. As of May 2012, 45% of enrolled subjects have at least one preserved PBMC specimen.

RNA Lab internal QC testing results

The TEDDY RNA Laboratory at Jinfiniti Biosciences in Augusta, GA (www.jinfiniti.com), has developed a high-throughput (96-well format) extraction protocol using magnetic (MagMax) beads technology (proprietary technology). Each plate of extraction contains 92 TEDDY samples, two positive control samples prepared by the TEDDY RNA Laboratory and two negative controls [phosphate buffered saline (PBS) buffer]. To assess the quality and quantity of the isolated RNA samples from whole blood and to monitor potential degradation over time, the lab has adopted a series of QC procedures. For each extraction plate, all 96 RNA samples are analysed using a spectrophotometer (NanoDrop) at 260 and 280 nm to document RNA concentration and quality in each sample. These concentrations are plotted in the TEDDY RNA Laboratory Information Management System, and negative control samples are used to assess potential cross-contamination during the entire process. The concentrations for the positive controls are compared with historical data for samples obtained from the same positive control individual, and these data are used to assess the overall quality of the extraction run. Failure of positive controls as well as TEDDY samples indicates technical problems associated with the run. A 260/280 nm ratio is calculated for each sample to assess the quality of the RNA samples. Ratios above 2.3 or below 1.6 are indications of poor quality and are flagged in the TEDDY RNA Laboratory Information Management System. The frequency and distribution of poor quality samples are calculated for every 12 consecutive plates (1104 samples) to assess technical and biological variation over time. Two TEDDY samples (one low and one high concentration) are also randomly selected from each plate to be analysed by the Agilent 2100 BioAnalyzer. Samples from every 12 plates are batched for a BioAnalyzer run. Once a year, 24 TEDDY RNA samples (11 fresh samples, 11 samples stored at -80°C for 6–12 months and two of the samples from pools of RNA from positive controls that have been created) are analysed by real-time reverse transcription polymerase chain reaction (RT-PCR) to assess the quality of RNA using several different genes (CDK2, GAPDH and HPRT1). Annually, 12 TEDDY RNA samples are analysed by microarray to assess their quality. On average, the total

RNA isolated is 10.8 μg with an average 260/280 nm ratio of 2.07. No significant degradation of the RNA has been observed over 3 years, and longer term stability is being monitored.

The TEDDY study has collected 2.5 mL of peripheral blood to extract total RNA from children enrolled in the study on the basis of the visit schedule outlined previously and in Table 1. As of May 2012, 73% of the one or more persistent autoantibody positive subjects have mRNA samples available. These samples have been allotted for gene expression studies.

Infectious agents

Many prior studies have linked viruses to both autoimmunity and T1D [10–12]. Thus, it is of great importance that the capture, processing and detection of infectious agents provide an optimum measurement and identify a valid exposure.

Preservation of enteroviruses in stool samples during shipment

Stool samples are collected from all TEDDY children starting at 3 months of age for virological and other microbiological analyses. Samples are taken at home by the parents and sent to the TEDDY Repository by express mail (US centres) or to the local repository by regular mail (European centres) where exposure to ambient temperatures for 1–3 days is possible. The effect of exposure to varying temperatures on enterovirus detection was evaluated by spiking enterovirus-negative stool samples or sterile water samples with infective enterovirus (Coxsackievirus B3) and then exposing them to different temperatures for 8–72 h. The varying temperatures evaluated were as follows: $4.0^{\circ}\text{C}/39.2^{\circ}\text{F}$, $25.0^{\circ}\text{C}/77.0^{\circ}\text{F}$, $35.0^{\circ}\text{C}/95.0^{\circ}\text{F}$, $43.0^{\circ}\text{C}/109.4^{\circ}\text{F}$, $56^{\circ}\text{C}/133^{\circ}\text{F}$ and $65.0^{\circ}\text{C}/149.0^{\circ}\text{F}$, at 8, 24, 48 or 72 h.

The preservation of enterovirus RNA was first analysed in spiked water samples by a sensitive semi-quantitative RT-PCR (5). The amount of viral RNA remained stable at temperatures $\leq 35^{\circ}\text{C}/95^{\circ}\text{F}$ for all tested time points. However, exposure to temperatures $\geq 43^{\circ}\text{C}/109^{\circ}\text{F}$ decreased the level of viral RNA detected, especially when exposed for 24 h or longer. The highest temperatures ($56^{\circ}\text{C}/133^{\circ}\text{F}$ and $65^{\circ}\text{C}/149.0^{\circ}\text{F}$) rapidly decreased the amount of viral RNA even after the shortest (8 h) exposure. The results were similar for the spiked stool samples.

The preservation of viral infectivity was analysed by plaque assay (the number of plaque forming units in green monkey kidney cells). Exposure to temperatures $\geq 56^{\circ}\text{C}/133^{\circ}\text{F}$ led to a rapid and complete loss of infectivity at 8 h exposure. Exposure to $43.0^{\circ}\text{C}/109.4^{\circ}\text{F}$ for durations < 72 h reduced infectivity by 50–80% and durations ≥ 72 h

led to a complete loss of infectivity. Exposure to temperatures ≤ 25.0 °C/77.0 °F did not reduce infectivity even after 72 h.

Overall, exposure to temperatures exceeding 35 °C/95 °F decreased both viral RNA and viral infectivity, and higher temperatures (56 °C/133 °F or higher) inhibited sensitive detection. Conversely, viral RNA and infectivity remained stable at lower temperatures. These findings resulted in the use of ice gel stool sample shipments during the summer months to eliminate deleterious temperature peaks. The maximal temperature to which the samples were exposed during regular ice gel packed shipments was monitored using commercially available CelsiStrip® temperature recording labels. Change in the colour indicated the maximal temperature of exposure. These stickers were placed inside the stool sample mailing box during summer months in 1467 shipments; the majority of samples (99%) remained at a temperature < 40 °C/105 °F.

Monitoring cross-contamination in TEDDY blood and stool samples

This QC protocol regularly monitors possible contamination of virus-negative samples by virus-positive samples (cross-contamination). This can happen when many samples are processed at the same time in the same location (e.g. when sample aliquots are made at TEDDY sites). Per protocol, sterile PBS samples are processed on a monthly basis in the same location as clinical samples. Possible contamination is then monitored by detecting enterovirus and rotavirus in these samples using sensitive RT-PCR. These viruses are common in children and are therefore optimal markers for contamination risk. PBS samples are processed in all sites that process blood, serum, plasma or stool samples in open tubes (e.g. dividing samples into smaller aliquots by pipettes or processing stool samples from diapers). PBS is first poured from a 500 mL bottle into a 50 mL tube in the same table or laminar flow where the samples are processed and divided further into 10 aliquots using the same procedures and equipment as for clinical samples. Samples are then shipped to the TEDDY Repository and stored at -80 °C. Samples are analysed regularly for the presence of rotavirus and enterovirus at the University of Tampere, Medical School (Tampere, Finland) using established RT-PCR methods validated in external QC rounds (QCMD; <http://www.qcmd.org> or equivalent). If needed, the samples can also be screened for other infectious agents. To date, 492 samples have been tested, and all have been virus negative.

Viral and pathogen detection using nasal swabs

This pilot study evaluated the validity of identifying respiratory viruses and other pathogens using nasal

swabs. Previous studies have found that nasal swabs are as effective as throat swabs for collecting samples from subjects with active upper respiratory infection; however, these methods have not been applied in regular sampling of asymptomatic subjects. Nasal swab sampling may be a non-invasive way to survey agents frequently causing infection and fever during childhood and the prevalence in the community during defined periods.

Samples were collected using Copan nasal swabs from 50 healthy subjects (age 1.5–14 years, 23 March to 1 April 2009) and 40 subjects with active upper respiratory tract infection (age 0.5 years–adults, 28 May to 5 November 2009). All subjects were from Turku, Finland. Laboratory analyses were performed using virus-specific PCR assays (RT-PCR) and multiple pathogen detection (multiplex PCR). For purposes of comparison, RT-PCR was performed at two independent sites in Finland (National Institute of Health and Welfare in Finland and University of Tampere, Finland). Multiplex PCR was performed at a third independent laboratory (Columbia University, New York) [13]. Results from all laboratories confirmed that respiratory pathogens can be detected using nasal swab procedures. The most frequently identified pathogens were human rhinovirus (HRV), *Haemophilus influenzae* and *Streptococcus pneumoniae*. Viral pathogens were more frequently reported in subjects with active upper respiratory infection than in healthy individuals (HRV: 26/9 versus *H. influenzae*: 15/2, *S. pneumoniae*: 2/6). Test accuracy was evaluated by false positive rates (FPR) and false negative rates. Using single pathogen detection in at least one lab to test subjects for clinical infections resulted in an FPR as high as 46/100 and a false negative rate of at least 22/100. However, estimating the frequency of asymptomatic and infectious subjects based on detection of multiple pathogens resulted in confirmed pathogen detection in 30/100 subjects with a low FPR of 6/100. Comparison of results across all three laboratories showed a high level of concordance with respect to HRV results. Confirmed positive HRV was detected in 65/100 symptomatic subjects with an FPR of 14/100. The virus-specific PCR assay had an overall concordance rate of 98/100 for HRV. This assessment confirms that viral and bacterial pathogens can be detected using nasal swabs in both symptomatic and asymptomatic subjects.

Beginning at 9 months of age, a minimally invasive nasal swab sample is collected from each TEDDY subject and continues to be collected on the visit schedule as outlined in the Study Design and Population Section. Nasal swab collection began in December 2008, and 67% of the enrolled cohort have available samples for analysis.

HbA_{1c} methods and quality control

The longitudinal design of TEDDY provides an ideal cohort to assess metabolic biomarkers and their utility in diagnosis and prediction. HbA_{1c} values reflect a 90-day moving average of blood glucose concentrations, weighted more heavily towards the last 30 days. The TEDDY HbA_{1c} samples are processed at the Diagnostic Diabetes Laboratory (Columbia, Missouri). The instrument Tosoh G7 HPLC analyzer, used for the measurement of HbA_{1c}, is calibrated using two whole blood calibrators – PLC and PHC Lot #4 (PLC4 and PHC4) using the target values that are accepted on the basis of the National Glycohemoglobin Standardization Program (NGSP) network reference. The same set of calibrators is used for the TEDDY study. As newer instruments are introduced, the instruments will be certified as secondary reference laboratory (SRL) methods for the NGSP before it can be used for routine analysis of clinical specimens. In addition, the laboratory participates in the College of American Pathologists GH2 survey twice a year as well as in the International Federation of Clinical Chemistry HbA_{1c} monitoring programme. Two samples are analysed each month. Furthermore, the laboratory also participates in NGSP Network Monthly Monitoring every month using the Ultra 2, Tosoh G7 and G8 HPLC methods, which are NGSP SRL methods. Monthly surveys are administered by the Central Primary Reference Laboratory (CPRL) to monitor performance of the network laboratories. Each month, the CPRL ships 10 specimens (fresh or fresh/frozen whole blood) over the desired clinical range (4–10% HbA_{1c}) to each network laboratory. The CPRL, PRLs and SRLs analyse the specimens in two separate runs on two separate days. All data are sent to the NGSP Administrative Core for analysis. To maintain certification, a network laboratory must fulfil the following bias and precision requirements: (1) the mean of the differences ($n = 10$) between the network laboratory and the CPRL must not exceed 0.35% HbA_{1c} and (2) the estimate of the standard deviation of the difference in sample replicates must not exceed 0.229 (99th percentile of the sampling distribution around a target SD of 0.15). SRL results must also fall within a defined acceptance ellipse based on the slope and intercept of the differences between the individual SRLs results and the medians of all SRLs.

The TEDDY study collects a whole blood sample for HbA_{1c} testing on children who are autoantibody positive starting as early as their 12-month visit and then every visit thereafter. TEDDY began HbA_{1c} collection in April 2009. Of the antibody-positive children, 55% have samples available.

TEDDY sample management

As described in Figure 1, the oversight and coordination of sample management, shipment and accountability are

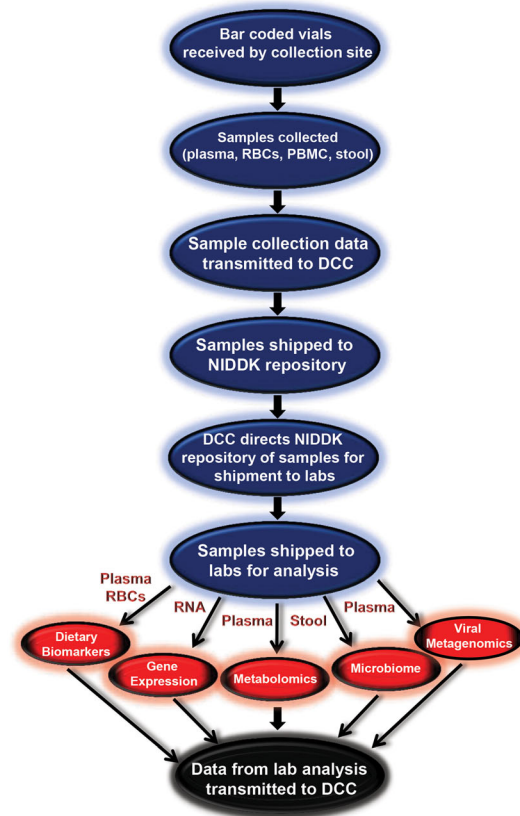


Figure 1. Outline of patient sample management for TEDDY. An overall flow chart details the organizational procedure for handling of various patient samples in terms of collection, shipment, analysis and record keeping. DCC, Diabetes Coordinating Center

directed by the DCC. Prior to collection of various patient samples, the DCC directs the shipment of appropriate storage containers to the various patient collection sites. All samples are aliquoted into dedicated, bar-coded (Symbol LS 2208) and colour-coded cryovials as determined by the type of particular analyses to be performed by selected laboratories. Each cryovial has a distinct and unduplicated barcode with a colour-coded top that allows for identification, tracking and differentiation among the thousands of samples collected. In addition, to promote the longevity of the samples obtained, preservatives are added at the collection stage to enhance long-term stability of the particular analyte. For example, plasma samples assayed for ascorbic acid analysis contain 0.2 mL of 5% trichloroacetic acid and 200 mg disodium EDTA/L. To preserve fatty acid analysis, collected erythrocytes contain 2 mL of 2-propanol with 50 mg/L of butylated hydroxytoluene. Following collection of patient samples, data are transmitted to the DCC containing all relevant information regarding the sample collected including barcode, sample type, sample volume, cryovial appearance, date of collection and patient information. Following

transmission of data to the DCC, the information is evaluated for potential errors and subsequently stored. The patient samples are then shipped frozen to the TEDDY Repository and immediately stored at -80°C . On the basis of the format of the experimental procedure, the DCC generates a list of required samples (patient and QC) for necessary analyses and transmits that information to the TEDDY Repository. The TEDDY Repository then removes those samples from storage, confirms the barcode and content and then ships to the selected laboratory for experimental analysis. All data files including initial raw data and modified datasets generated by the selected laboratories are transmitted and stored at the DCC.

The DCC has compiled samples strictly for QC purposes that have been incorporated into the overall sample management (Figure 1) to measure and determine inter-assay and intra-assay variability from the data received from the various selected laboratories. These QC samples appear identical and similar in biological nature to actual patient samples. Therefore, these samples (plasma, red blood cells, stool, RNA and infectious agents) are processed in the same manner and are stored in sample-matched bar-coded vials. Also, pseudo patient IDs and site visits are incorporated for each QC sample to mimic actual patient samples and prevent the laboratory from distinguishing QC samples. QC samples are then integrated into DCC-established experimental design and prepared by the DCC QC laboratory and shipped to the TEDDY Repository for storage at -80°C . QC samples are then integrated into the patient sample sets sent to the core laboratories for analysis as previously described (Figure 1). Data generated from the analysis of these QC samples are sent to the DCC as described for patient samples.

Data collection and analysis

With over 250 million data points collected thus far, the QC methods employed throughout the collection, entry and management of TEDDY data are of paramount importance to the overall integrity of the study.

Data are extracted by trained staff members during scheduled visits and entered directly via standard forms (Web forms or through teleforms), which are scanned and transmitted electronically. Front-end constraints are employed in the Web application to prevent the entry of invalid data; for example, certain fields are required, only valid dates may be entered and ages must fall within a predefined range. All TEDDY data are stored in fully managed Oracle databases at the DCC and archived regularly, both on-site and off-site, to ensure data security. In addition to the front-end constraints applied at the time

of entry, a unique automated QC system has been developed for the TEDDY project.

The TEDDY Error Reporting and Verification System (ERVS) consists of a set of programmes that conduct automated QC on TEDDY data, a specialized Web application for reporting and resolving errors, an integrated database for storing error data and a set of programmes that generate reports for monitoring data cleaning efforts. Manifold error checks are conducted as a part of this automated QC processing. These include, for example, comparing dates against the visit date, the subject's birth date and the current date; checking answers to responses on related questions for conflict; identifying outliers through a variety of techniques particular to the circumstance; and verifying all codes using existing code databases. Any detected errors are stored in the ERVS database and are automatically available through the Web application. Staff members at the clinical centres then use the Web application, along with the original article records stored at their site, to correct or verify all reported errors. The process is monitored and directed throughout by using extensive ERVS summary reports that detail the number of errors identified, pending, corrected and verified across clinical centres, forms and even individual questions.

The ERVS allows for timely and directed data cleaning while reducing the burden on both the clinical centres and the DCC. The process is automated and standardized and has resulted in a significant acceleration in manuscript development. Real-time QC processing enables the immediate identification of data collection or entry issues. This assists in maintaining the interpretation of the MOO and allows for targeted retraining of staff, both essential to maintaining data integrity in a massive, multinational and longitudinal study. Critically, the ERVS has resulted in the correction or verification of 117, 545 data entry errors; a relatively small (0.28%), but nonetheless significant, portion of the total number of data points checked.

The Environmental Determinants of Diabetes in the Young analyses data are further subjected to external QC as a part of the data sharing process. Raw manuscript datasets are submitted to the NIDDK Data Repository where they undergo a 'Dataset Integrity Check'. The Dataset Integrity Check is conducted by NIDDK-affiliated statisticians who independently replicate the published results using the raw datasets provided.

Discussion

The TEDDY project represents a unique and massive undertaking to unravel critical clues towards the elucidation of the causative mechanisms of T1D. Because of the multifactorial nature of this disease, it has become necessary to

Table 2. Detailed summary of quality control and availability of biospecimens (sample availability current as of May 2012)

Biospecimen	Quality control	Final product	Sample availability in cohort or nested case-control
Peripheral blood mononuclear cells (PBMC)	Blood collection from TEDDY Manual of Operations with certified technicians followed by cell viability assay	Recovery of cells maintenance of good viability, functionality control (mean recovery >60% and >90% viability) – 5–10 × 10 ⁶ PBMC/mL/2–5 vials per subject	45% cohort
Human leukocyte antigen	Proficiency tested whole blood and dried blood spots samples with a wide range of validated HLA-DR and HLA-DQ genotypes	99% accuracy in identifying relevant HLA-DR or HLA-DQ alleles	100% cohort
Diabetes autoantibodies	Concordance of GADA and IA-2A retested by two laboratories	Concordance with harmonized assay for GADA is 98.2% and 97.3% for IA-2A. The harmonized assay is used for TEDDY protocol.	78% cohort
Transglutaminase autoantibodies (tGA) Infectious agents – enterovirus	Interlaboratory tGA assay concordance Preservation of enterovirus after exposure to varying temperatures and periods during stool sample transport using reverse transcription polymerase chain reaction in spiked water samples	93% concordance between two tGA assays At +4 °C/39 °F and +25 °C/70 °F both RNA and infectivity preserved for 72 h. Samples per protocol will not be exposed to temperatures of 43 °C/110 °F or higher. Ice gel is now included in the TEDDY stool sample shipments during the hot summer months to eliminate deleterious temperatures peaks.	100% starting at 24 months of age 81% enterovirus antibodies and polymerase chain reaction – case-control
Infectious agents – nasal swabs	False positive and false negative rates of virus/pathogen detection; frequency of asymptomatic and infectious subjects with multiple viruses or pathogens; and concordance of sample results across three labs	Respiratory pathogens can be frequently detected in nasal swabs using both multiplex and pathogen-specific molecular methods.	67% cohort
mRNA	Absorbance 260/280 followed by Agilent 2100 BioAnalyzer	High quality 10.6 ug/blood sample stored for gene expression studies	73% case-control
Glycated haemoglobin (HbA _{1c})	Certification maintained through the National Glycohemoglobin Standardization Program Administrative Core	The mean of the differences in samples (n = 10) between the network laboratory and the Central Primary Reference Laboratory must not exceed 0.35% HbA _{1c} and the estimate of the standard deviation of the difference in sample replicates must not exceed 0.229 (99th percentile of the sampling distribution around a target standard deviation of 0.15). Coefficient of variation < 1.3%.	55% autoantibody positive subjects in TEDDY cohort

collect a multitude of specimens longitudinally from numerous centres. This has posed serious challenges in QC. The solution entails multiple QC steps for each data point and specimen collection with continual evaluation of archived samples. In doing so, TEDDY has built a generous repository that can serve as the basis for a multitude of studies understanding the determinants responsible for T1D (Table 2). The robust QC effort should greatly enhance the value of the samples and data collected by TEDDY as a key resource to investigators proposing innovative hypotheses concerning candidate environmental and genetic factors.

Acknowledgements

The TEDDY Study Group (see online appendix) is funded by U01 DK63829, U01 DK63861, U01 DK63821, U01 DK63865, U01 DK63863, U01 DK63836, U01 DK63790, UC4 DK63829, UC4 DK63861, UC4 DK63821, UC4 DK63865, UC4 DK63863, UC4 DK63836, UC4 DK63790 and UC4DK095300 and contract no.

HHSN267200700014C from the National Institute of Diabetes and Digestive and Kidney Diseases (NIDDK), National Institute of Allergy and Infectious Diseases (NIAID), National Institute of Child Health and Human Development (NICHD), National Institute of Environmental Health Sciences (NIEHS), Juvenile Diabetes Research Foundation (JDRF) and Centers for Disease Control and Prevention (CDC).

Conflict of interest

The authors have no conflicts of interest. If any material presented in this manuscript has been published elsewhere, it is appropriately cited.

Supporting information

Supporting information may be found in the online version of this article.

References

1. The TEDDY Study Group. The Environmental Determinants of Diabetes in the Young (TEDDY) study. *Ann N Y Acad Sci* 2008; **1150**: 1–13.
2. Hagopian WA, Erlich H, Lernmark A, *et al.* The Environmental Determinants of Diabetes in the Young (TEDDY): genetic criteria and international diabetes risk screening of 421 000 infants. *Pediatr Diabetes* 2011; **12**(8): 733–743.
3. Kiviniemi M, Hermann R, Nurmi J, *et al.* A high-throughput population screening system for the estimation of genetic risk for type 1 diabetes: an application for the TEDDY (the Environmental Determinants of Diabetes in the Young) study. *Diabetes Technol Ther* 2007; **9**: 460–472.
4. Erlich H, Valdes AM, Noble J, *et al.* HLA DR-DQ haplotypes and genotypes and type 1 diabetes risk: analysis of the type 1 diabetes genetics consortium families. *Diabetes* 2008; **57**: 1084–1092.
5. Dantonio P, Meredith-Molloy N, Hagopian WA, *et al.* Proficiency testing of human leukocyte antigen-DR and human leukocyte antigen-DQ genetic risk assessment for type 1 diabetes using dried blood spots. *J Diabetes Sci Technol* 2010; **4**: 929–941.
6. Bonifacio E, Yu L, Williams AK, *et al.* Harmonization of glutamic acid decarboxylase and islet antigen-2 autoantibody assays for national institute of diabetes and digestive and kidney diseases consortia. *J Clin Endocrinol Metab* 2010; **95**: 3360–3367.
7. Li M, Yu L, Tiberti C, *et al.* A report on the International Transglutaminase Autoantibody Workshop for Celiac Disease. *Am J Gastroenterol* 2009; **104**: 154–163.
8. Immune Tolerance Network. Isolation and cryopreservation of PBMC. CPT without Plasma Collection [v. 009], 2006.
9. Mallone R, Mannering SI, Brooks-Worrell BM, *et al.* Isolation and preservation of peripheral blood mononuclear cells for analysis of islet antigen-reactive T cell responses: position statement of the T-Cell Workshop Committee of the Immunology of Diabetes Society. *Clin Exp Immunol* 2011; **163**: 33–49.
10. Tauriainen S, Oikarinen S, Oikarinen M, Hyoty H. Enteroviruses in the pathogenesis of type 1 diabetes. *Semin Immunopathol* 2011; **33**: 45–55.
11. Oikarinen S, Martiskainen M, Tauriainen S, *et al.* Enterovirus RNA in blood is linked to the development of type 1 diabetes. *Diabetes* 2011; **60**: 276–279.
12. Stene LC, Oikarinen S, Hyoty H, *et al.* Enterovirus infection and progression from islet autoimmunity to type 1 diabetes: the Diabetes and Autoimmunity Study in the Young (DAISY). *Diabetes* 2010; **59**: 3174–3180.
13. Briese T, Palacios G, Kokoris M, *et al.* Diagnostic system for rapid and sensitive differential detection of pathogens. *Emerg Infect Dis* 2005; **11**: 310–313.